TECHNICAL INSTRUCTIONS

tempo®

FEATURING:

- Intelliweave™ composite
- Service Free Design
- High Weight Limit

PACKAGE CONTENTS	TOOLS RECOMMENDED
(1) Tempo Foot, with Bonded Foot Shell	4mm Hex Key

college park
technology for the human race

WARRANTY INSPECTION AND MAINTENANCE INFORMATION

College Park recommends that you schedule your patients for check-ups according to the warranty Inspection schedule below.

High patient weight and/or impact level may require more frequent inspections. We recommend you visually inspect the following applicable parts for excessive wear and fatigue at each warranty inspection.

- Composites and Adapters
- Foot Shell

WARRANTY INSPECTION SCHEDULE FOR TEMPO: ANNUALLY.

TECHNICAL ASSISTANCE / EMERGENCY SERVICE 24-7-365

College Park's regular office hours are Monday thru Friday, 8:30 AM – 5:30 PM (EST). After hours, an emergency Technical Service number is available to contact a College Park representative.

college park
800.728.7950 | 586.294.7950 | college-park.com

MADE IN THE USA
311 INS TO TIS 150119 CE

COLLEGE PARK INDUSTRIES
27955 College Park Dr. Warren, MI 48088 USA

EC REP **EMERGO EUROPE**
Molenstraat 15, 2513 BH, The Hague, Netherlands

©2016 College Park Industries, Inc. All rights reserved. College Park and Gait Matching are registered trademarks of College Park Industries. Horizon, FootHorn and CPI Sock are trademarks of College Park Industries.

FOOT COMPONENTS

This diagram is to help familiarize you with the unique parts of the Tempo. These parts are referenced in the instructions and used when speaking with a technical service representative.

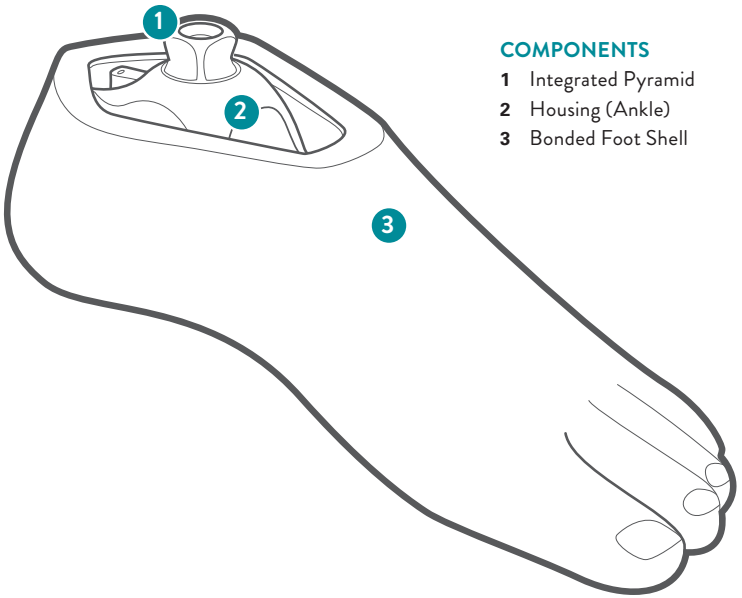

COMPONENTS

1 Integrated Pyramid
2 Housing (Ankle)
3 Bonded Foot Shell

⚠ WARNING

- Do not expose this product to pH extremes or corrosive materials (water, salt water or other liquids).
- Failure to follow these technical instructions or use of this product outside the scope of its Limited Warranty may result in injury to the patient or damage to the product.
- Disassembly, modification or removal from the foot shell, or any further disassembly or modification of components will void the warranty.

GENERAL INSTRUCTIONS

MOUNTING

Use only high quality proximal endoskeletal components (30 mm). The service-free Tempo foot comes permanently assembled in the foot shell.

STATIC ALIGNMENT

For optimal function have the patient's weight balanced between the forefoot and heel.
The load line divides the foot at the 1/3 heel lever and 2/3 toe lever.

DYNAMIC ADJUSTMENTS

DESIRED RESULT	ALIGNMENT CHANGE
Firmer Toe Response	Plantarflex the Tempo or move load line posterior
Softer Toe Response	Dorsiflex the Tempo or move load line anterior
Firmer Heel Response	Dorsiflex the Tempo or move load line anterior
Softer Heel Response	Plantarflex the Tempo or move load line posterior

GAIT MATCHING® GUIDELINES

Contact College Park Technical Service if you have questions about modifying the gait match.